


SYSTEM DIAGRAM

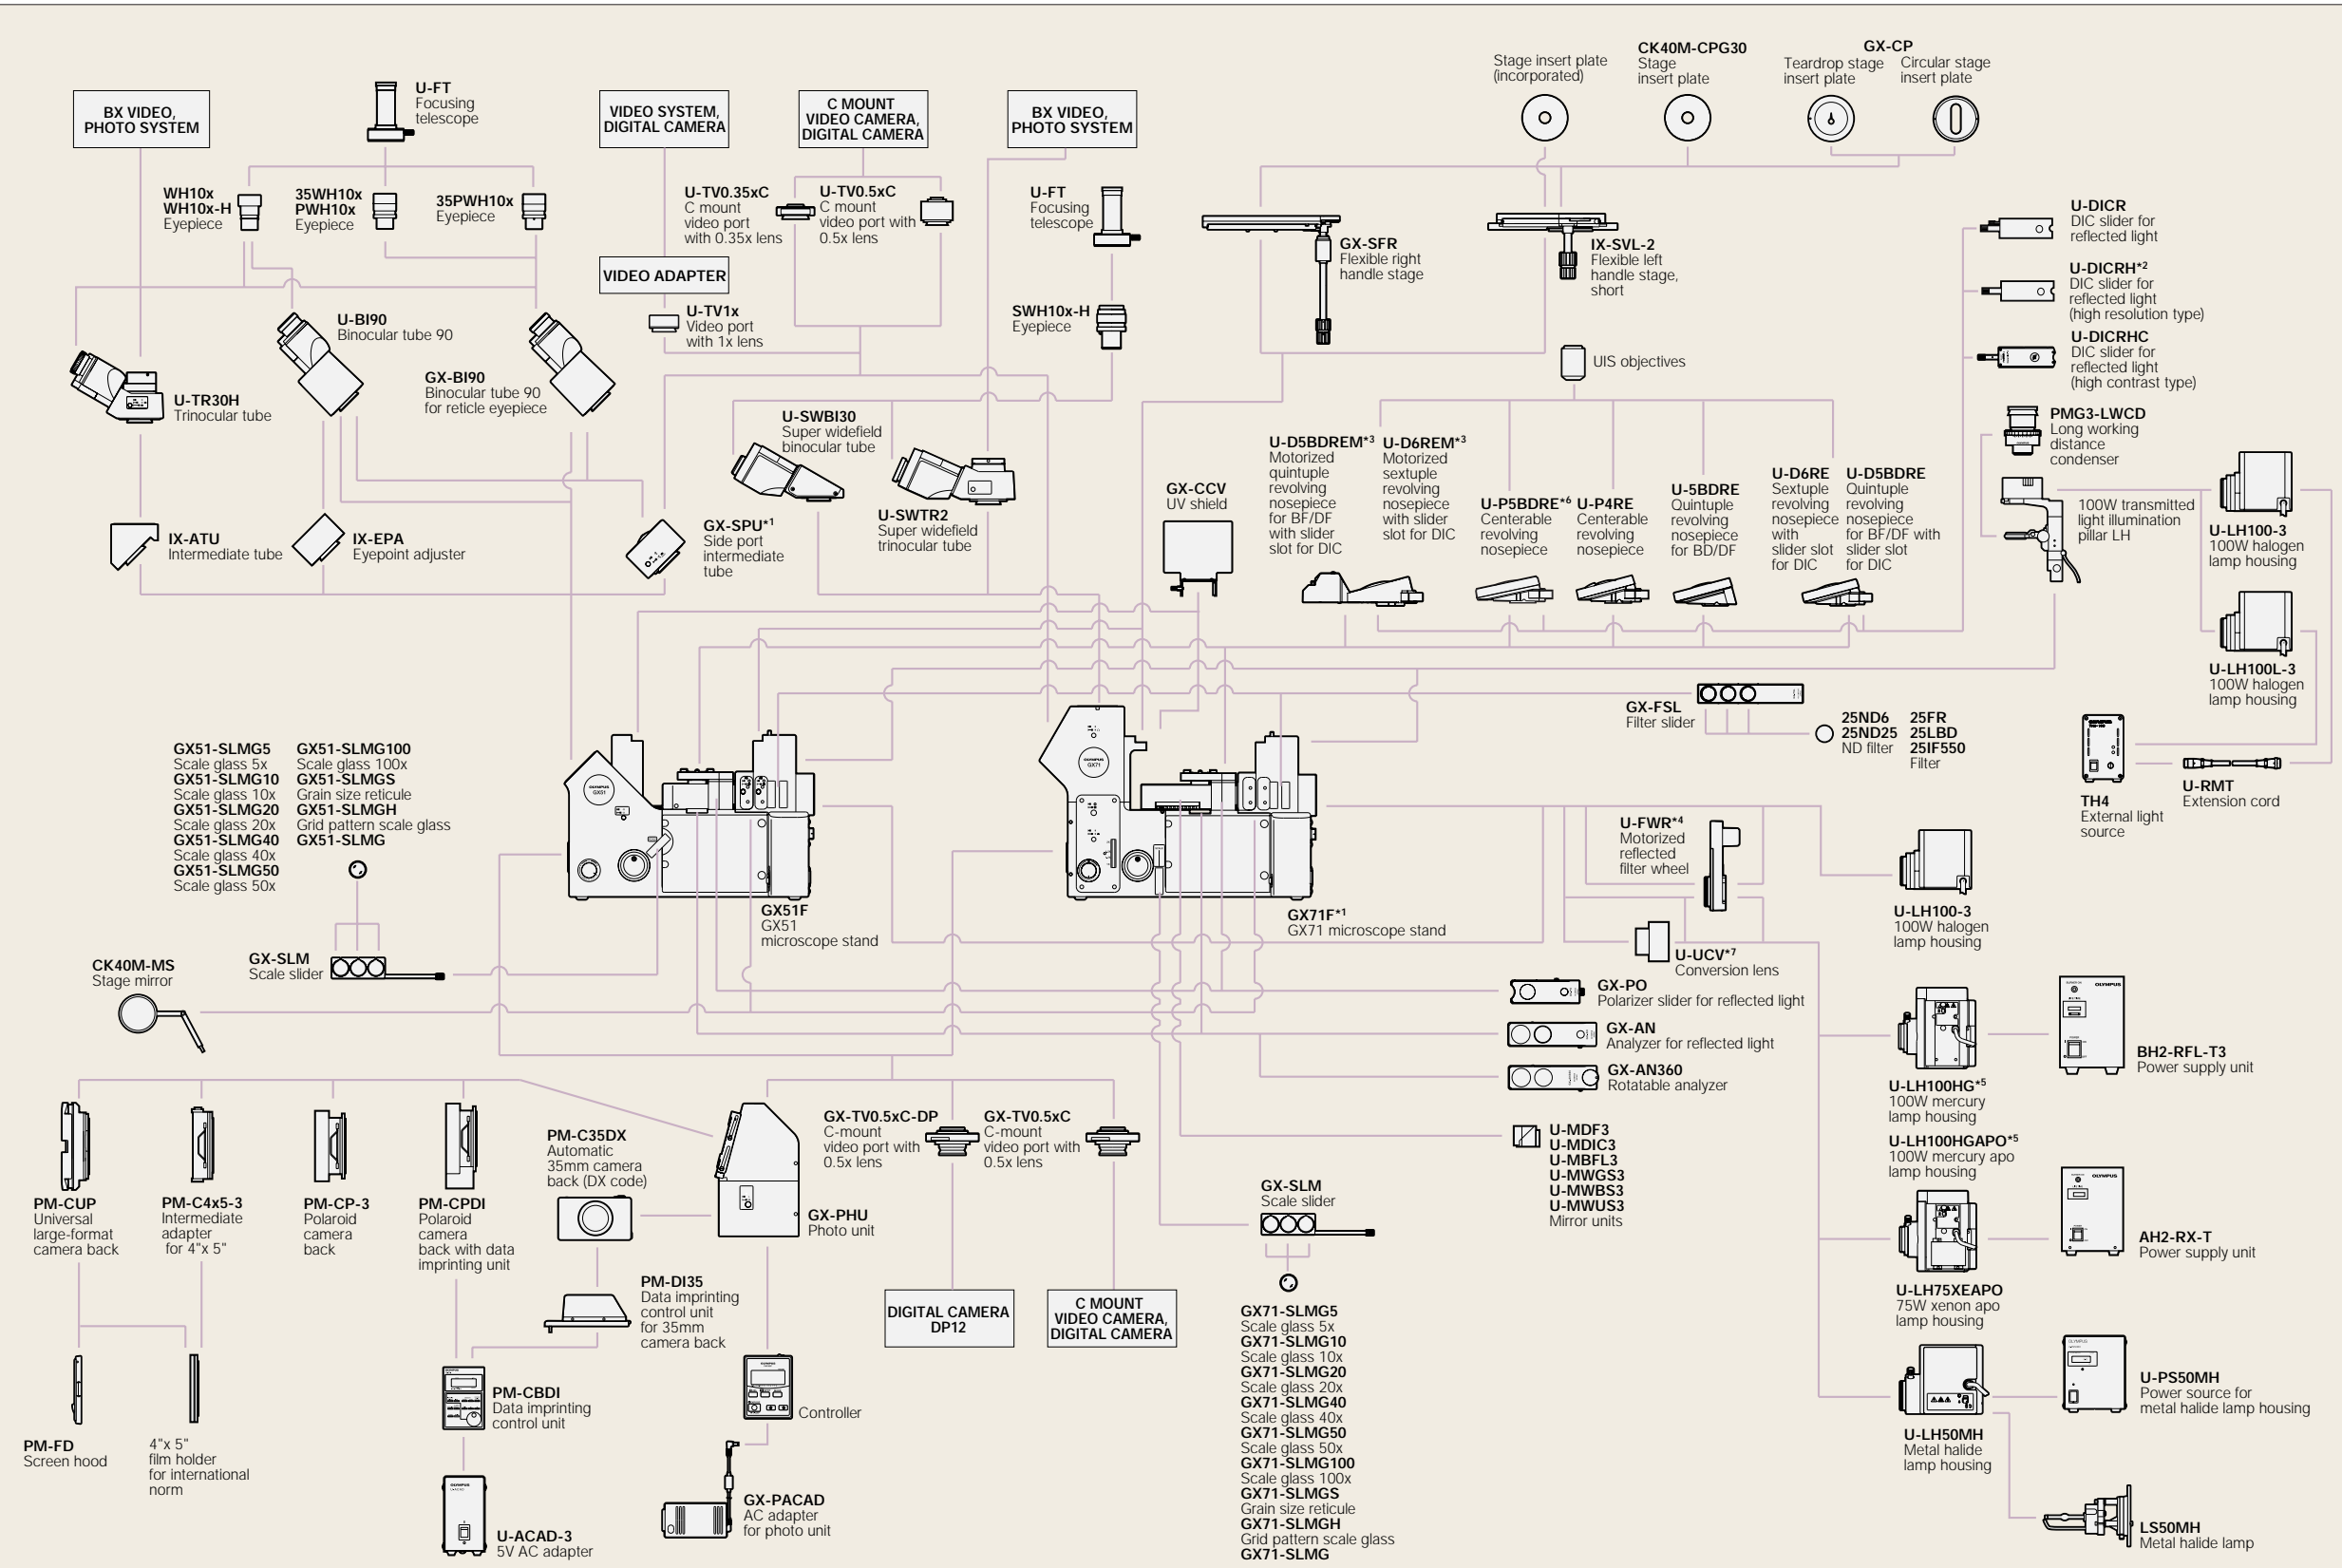

*1 Please consult your nearest Olympus dealer for cameras compatible with the GX71F side port and GX-SPU. The PM series photomicrographic system cannot be attached. *2 Sensitive tint observation cannot be accomplished with U-DICRH. *3 U-REMP-2 power supply unit is required for U-D6REM and U-D5BDREM. *4 IX-UCB control unit is required for U-FWR. *5 25L42 filter is needed for polarized light and Nomarski DIC observation using high intensity lamps such as U-LH100HG. *6 Objectives may touch the stage when revolving the U-P5BDRE incorrectly. *7 U-UCV can be used in for fluorescence observation.